

BioGen Technologies INC

User Manual

Say Hello To Wellness

This Device Is Not For Use On Clients With Pacemakers.
Please Use With Medical Surge Protector Only.

The I.M.A.E.T. System
Immune Modulation & Allergy Elimination Technology ^{TM/A}

BioGen Technologies

The Future Is Today

I.M.A.E.T. System

This Entire Program
Is Copyright Protected
By International Law
2001-2008 ©

Presents

The I.M.A.E.T. System TM

Modern Biofeedback Technology

Copyright 2008

Revision: 11/2012

Table of Contents

Topic	Page #
Mission Statement	1-A
About Program & Quick Start Summary	2-A, B, C
Wellness Info & Function Panel	3-A, B
Demographics Profile	4-A, B
Lifestyle & Calibration Panel	5-A, B
History Profile	6-A
Reactivity Test Panel	7-A, B, C
Chiropractic Panel (Spinal & Dermatome Profile)	8-A, B
Neuro-Emotional Profile	9-A, B
Acupuncture-TCM Panel (Meridian Profile)	10-A, B
Chromosome, Gene & Cell-Com	11-A, B
Organ-Specific Sarcodes	12-A, B
Color, Chakra & Aura Profile	13-A, B
Circulatory & Heart Profile	14-A, B
Lymph Profile	15-A, B
NAET Profile, Test Panel	16-A, B, C
Homeopathic Profile	17-A, B
Nutritional Profile	18-A, B
Hormone Profile	19-A, B
Neurology Panel / Brain Profile	20-A, B, C
Detox & Multiple Stress Profile	21-A, B
PetVibes/Animals Profile	22-A, B
System Specifications	23-A, B



Mission Statement

The Mission of BioGen Technoogies Inc is to produce the finest biofeedback, relaxation management instrument possible. Every component of the I.M.A.E.T. System has been compiled with the greatest degree of competency and integrity. Professionals and others interested in the exciting world of biofeedback and relaxation management may use the system as a bridge to aiding the body's own relaxation mechanisms.

Special attention was given to the application of the NAET procedures in this system. BioGen Technologies is dedicated to providing technical assistance, Internet web support and professional training.

[Please Note:](#) Questions, comments, suggestions and corrections are always welcome.

About This Program

The I.M.A.E.T. System software is protected by copyright and may not be duplicated, or copied, in any form, without written permission.

The I.M.A.E.T. System is a biofeedback, relaxation management instrument. No information should be construed as a medical claim or representation that this product is intended for use in the diagnosis, cure, mitigation, treatment, and prevention of disease or any other medical condition. A biofeedback, relaxation and stress management device records subtle, “reactive,” informational potentials provided by the client during the assessment procedure. The computer evaluates such responses, and then challenges the individual with that information by feeding it back to the client. This process assists the body’s own relaxation and stress management mechanisms by encouraging a sense of wellness, balance and harmony.

The interface box and harness are not intended for use on clients with pacemakers or other electrical devices. Disconnecting the interface box and utilizing the “Metaspace” mode may facilitate those clients with special needs.



Cable & Box Connections


Attach the USB interface cable, the 9-pin head harness cable and the 9-pin limb harness cable to the back of the I.M.A.E.T. System box. Attach the other end of the USB interface cable to the back of your computer, **ONLY AFTER THE SOFTWARE HAS BEEN INSTALLED, OR YOU ARE INSTRUCTED TO DO SO DURING THE SOFTWARE INSTALLATION PROCESS.**

Limb Harness Placement

The 4 limb harness bands may be applied to ANY wrist or ankle.

Head Harness Placement

Wrap snugly around head, with the 8 conductive vinyl strips in contact with the forehead. Secure at the back of the head with Velcro enclosure.

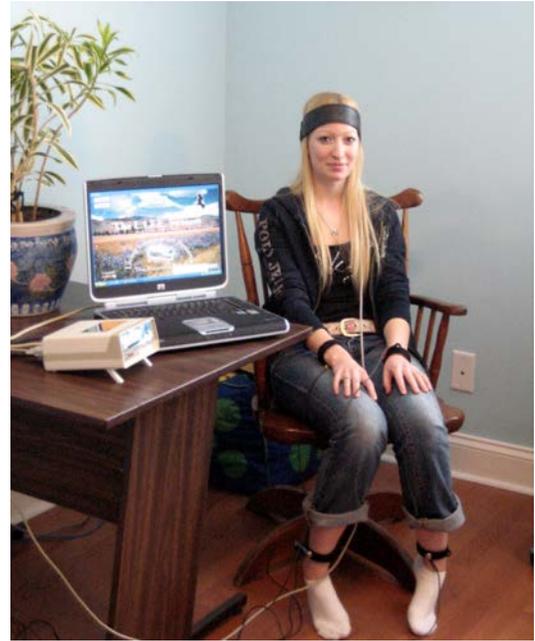

Quick-Start Summary

Please Note: The I.M.A.E.T. System software is a copyrighted program that is owned by Living Information Systems ^{LLC} and is licensed to the initial user under the terms and conditions specified in the Warranty, Sale and Software Installation Agreements. Resale to another party may incur a re-licensing fee, at the discretion of the software manufacturer. When using a laptop computer, it is suggested that you leave it plugged into the wall while using the I.M.A.E.T. System. The battery only feature of laptop computers prolongs the time it takes to process information during certain functions.

A typical combined assessment and feedback procedure should last approximately 1 hour, dependent upon: 1: the client interview, 2: type of information provided by the client, 3: the Body-Biofield **Reactivity** assessment, and 4: subsequent feedback procedures.

The following typical protocol is suggested:

Step 1: Open the program and click **Continue** upon opening the initial panel. This will bring you to the **Navigation** page. Next, type your password into the **Login** field. Then click **To Demographics** on the **Navigation** panel. Click **New Client** then Enter Name, Address, Phone number etc. and any other appropriate information you may wish to enter about your client. Click **Save All** before leaving.

Step 2: Proceed to the **Lifestyle Profile**, and enter the client's numerical responses, based upon each of the 20 questions posed. Do not enter percentages or letters, **only numbers**.

Step 3: Proceed to the [History Profile](#) by recording, checking and entering information into all appropriate fields. Now return to [Lifestyle Profile](#).

Step 4: Attach the head harness and the wrist & ankle straps to the client. Then click [Calibration](#). Upon completion, click save and proceed to step 5.

Step 5: Next, proceed to the [Wellness Info](#) panel. Click on the red [Wellness Info](#) button, and select one of the 16 programs offered there. It is on the [Wellness Info](#) page where you will find the [NAET](#) page, which will take you to the [NAET Profile](#).

Step 6: Click [To Body-Biofield Test](#) to initiate activation of the assessment process. This test is used to evaluate responses relevant to possible indications of stress and muscle tension. Click the “[Test Potential](#)” button to begin the process. Following an approximate 4 to 7 minute test, the most significant results and indications for relaxation feedback will be displayed in descending numerical order from top to bottom. A bar graph is also used to *graphically* display a significant response. These results may then be used as a guide for considering subsequent feedback procedures. A response of 75% or greater (on the graph), or 1500⁺ (in the numerical, “[Significance](#)” column), is considered appropriate for applying a feedback procedure. You may then select any item in the matrix by clicking and highlighting it and then clicking either the [5 Second Auto](#) or [Feedback–30 Seconds](#) button. An additional option would be to set the timer for the desired feedback duration, from 1 to 30 minutes, then select either the Harness or Metaspacer option.

Note: In order to get back to the NAET panel, please click on [Wellness Info](#)!

It is not recommended to do a [Body-Biofield](#) assessment and a NAET reactivity assessment on the same day / visit. Please do either / or and work with the information obtained for that day!! You can always come back another day and use the same results for another treatment.

Step 7: Based upon the information provided by all of the previous factors, the practitioner will go to [Wellness Info](#) to choose and apply the specific feedback procedures as indicated. Typical feedback procedures range from one to three minutes, or more, dependent upon individual assessment needs.

Step 8: Upon completion of feedback, results may be assessed through a brief, final interview with the client, to determine his/her sense of wellness and relaxation/stress reduction levels. Subsequent visits may be determined and scheduled in accord with the client’s personal and/or projected sense of well-being, as well as the practitioner’s observation.



Wellness Info & Function Panel

DO NOT USE THE HARNESS AND THE INTERFACE BOX ON CLIENTS WITH PACEMAKERS OR OTHER MEDICAL IMPLANT DEVICES OR COMPONENTS.

The [Wellness Info](#) page provides a user-friendly index and access to all programs and settings within the I.M.A.E.T. System. To activate the system for the first time, you will need to obtain an activation code from Living Information Systems support staff, prior to proceeding. Following this, your password must be entered into the [Navigation](#) page. If you are loading the program on more than one computer, you will need an activation code for each computer. This procedure will need to be implemented *only once for each computer*.

Function settings such as [EMR Protection](#) may be modified from this panel. While you may change the EMR setting, **it is strongly recommended that you use the default setting**, which allows for fulltime EMR protection.

The [Program Info](#) button opens a window to general instructions about the programs.

In order to enter a new client or select a previously saved client, you must click on the [To Demographics](#) button located at the bottom right of the [Wellness Info](#) screen.

YOU WILL RETURN TO THE “WELLNESS INFO” PANEL EACH TIME YOU MAKE A NEW PROGRAM SELECTION. When you choose to leave an active program panel, click the “[WELLNESS INFO](#)” button on that screen and you will return to this window, enabling you to make another selection. Should you choose to leave the entire program and return to the Windows Desktop, click the [Exit](#) button. **YOU MUST EXIT AND REOPEN THE PROGRAM EACH TIME YOU WORK WITH A NEW OR EXISTING CLIENT.**

Summary of Features:

- Turn off “EMR protection” (**NOT RECOMMENDED**)
- Go to “Lifestyle Profile”
- Go to “Demographics”
- Select any Program from the “Wellness Info” page

Demographics

[New Client](#) [Save All](#) [Rem. Client](#) ID: < Sort By

Member ID	Last Name	First Name	Member Type
1	Keiser	Chic	Human Male

Home Address:

City: State: Zip Code: Date Joined (m/d/y): 5/18/2005

Home Phone: Country:

Birthdate (m/d/y): Birthplace: Time of Birth:

Email Address:

Previous Visits

Date	Time	MR
4/5/2005	11:26:02 AM	MR
4/5/2005	11:58:37 AM	MR
4/5/2005	7:45:48 PM	MR
4/15/2005	5:39:08 PM	MR

[Follow-up Visit](#) [Remove Visit](#)

Work Company: Title:

Work Address:

City: State: Zip Code:

Work Phone: Country:




L.I.F.E. System

Client Affirmation
I am perfectly healthy and well in every way.

ID	LASTNAME
1	Keiser
2	Keiser
3	Binkethoff
4	Cain
5	Binkethoff

[Load Pic](#) [Client Picture](#) [Remove Pic](#)

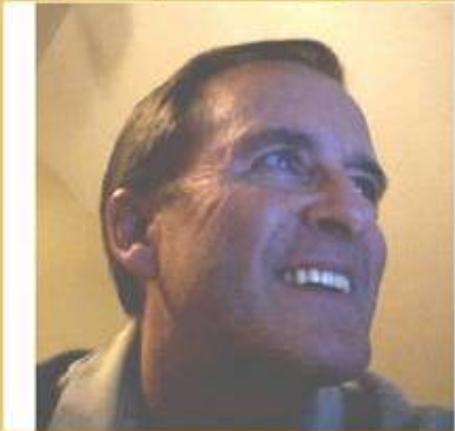

[Print Visit](#) [Program Index](#) [To History Profile](#)
[Restore Data](#) [About Panel](#) [Lifestyle Profile](#) [To Reactivity Test](#)

Demographics

The [Demographics](#) screen contains all the appropriate and pertinent information pertaining to your client. Click the [New Client](#) button at the top right of the screen. To ensure proper functioning of the device enter the last name, first name, gender of the person or pet, home address, city, state, zip/postal code, date, telephone number, country, birth date and birthplace. All other fields including the e-mail address, work or company name, title, work address, work phone and country are desirable, but NOT ESSENTIAL. To [delete a client](#), simply highlight the name in the client list, then click the [Rem. Client](#) button at the top left of the screen and [SAVE ALL](#). To [delete a visit](#) for a particular client, highlight a date in the [Previous Visits](#) list and click [Remove Visit](#). **NOTE:** you must click [Save All](#) at the top left of the screen following any entry. If you wish to [add a visit for an existing client](#), highlight the client's name in the client list, then click the [Follow-up Visit](#) button. A current date will be added to that client's record.

Inserting a [Personal Affirmation](#) and a picture of your client **IS HIGHLY RECOMMENDED**. The personal affirmation may be typed into the box under [Client Affirmation](#). It will automatically be stored with the rest of the information you enter into this panel upon clicking the [Save](#) button. The affirmation may be changed on subsequent visits. If the client supplies you with a picture it must be stored in the [Patient Pictures](#) file of the program and may be imported from a digital camera (recommended), CD, flash card or other image source. It is recommended that the practitioner purchase an inexpensive Digital camera, which can be utilized with a laptop or desktop computer for this purpose. It is not recommended that you use images transferred via the Internet as they may contain viruses. **BE CERTAIN ABOUT THE INTEGRITY OF THE SOURCE PICTURE.**

Click on the [Save All](#) button after entering the necessary demographic information. This will preserve and store the entries you have made. If you make [ANY](#) changes to the demographic data during subsequent sessions, be sure to save them before leaving.

The [Restore Data](#) button allows you to store and retrieve all your patient files in a backup folder in the event of a computer failure.

The [Print Visit](#) button allows you to select a date in the [Previous Visits](#) box and print the [Main Reactivity Test](#) that was stored for that visit.

If you are returning to the [Demographic](#) panel in order to select a previous client and you [ARE NOT](#) making any demographic changes or other entries, click and highlight the client's name in the alphabetical client list, then click the [Follow-up Visit](#) button, which will enable a new date and history index for an existing client. Next, proceed to the [Lifestyle Profile](#) panel.

Summary of Features:

- Enter demographic data for a new client
- Insert a personal affirmation and a picture of your client
- Save pertinent data for each new client
- Click the Follow-up Visit button for a returning client
- Print Main Reactivity Tests from here if appropriate
- Go to "Lifestyle Profile" page

Patient Name:
Smith John

Lifestyle Profile

Previous Visits

24/06/2008 12:08:45 AM
25/06/2008 1:49:33 AM
25/06/2008 6:55:00 AM

Have You Had Any Major Organs Removed? How Many?
 Do You Use Prescription Medications? If So, How Many?
 Do You Use Tobacco? If So, How Many Times Per Day?
 Have You Used Steroid Drugs In The Past Year? How Many?
 Do You Have Amalgam Fillings? If So, How Many Currently?
 If you Use Recreational Drugs, How Many In the Past 30 Days?
 Do You Have Any Debilitating Allergies? How Many?
 Do You Suffer From Emotional-Mental Conditions? How Many?
 Do You Accept Responsibility For Your Health? On Scale Of 1-10
 Estimate The Amount Of Fat In Your Diet. Enter Number 1 to 100

Do You Suffer From Personal Stress? Enter Number 0 to 10
 Do you Eat Sweets? Estimate # Per Day. Candy, Cola, Cake, Etc.
 Do You Exercise Weekly? How Many 15 Min Sessions Per Week?
 Do You Use Alcohol? If So, How Many Drinks Per Week -Average?
 Do You Ingest Caffeine? Include Coffee, Cola, Tea, Etc. # Per Day?
 Have You Been Exposed To Any Serious Toxins? How Many?
 Have You Had Any Major Infections In Your Life? How Many?
 Have You Had Any Major Injuries In Your Life? How Many?
 How Many Glasses Of Water Or Liquid Do You Drink Per Day?
 Do Your Feel That You are Over-weight? If So, How Many Pounds?

Calibration

Start Calibration

Lifestyle & Calibration Profile

If you have already completed the Demographic screen, you will notice the name of your client appears in a field at the upper left corner of the [Lifestyle Profile](#).

Interview the client, using the questions supplied, and enter an appropriate number in each of the boxes. **Do not enter zero's, letters or % signs in any of the fields, just numerals.** Make sure that the "Save" button is clicked following completion.

Questions posed in this panel are generic and do not represent a medical profile. The information is gathered in order to help the client and the practitioner understand what processes inhibit the client's overall well-being or lifestyle. Information should be reviewed with the client on subsequent visits to ascertain whether that individual is striving to make changes that will influence his/her state of relaxation/wellness. Information from this profile will be saved to a dated file that is linked to the [Previous Visits](#) box above. Clicking on a date in the [Previous Visits](#) box displays data for the selected visit.

At this time, place the head and limb harnesses into position on your client, unless you are using the Metaspacer function. **WARNING: YOU MUST USE THE METASPACE FUNCTION FOR CLIENTS WITH PACEMAKERS. DO NOT USE THE HARNESS SYSTEM On Patients with pacemakers or defibrillators.**

You may now proceed with the Quad-mode Entrainment [Calibration](#) process.

Make sure that you have attached the head and limb harnesses, then click the red [Start Calibration](#) button. Calibration attunes the individual by creating a link between the individual and the IMAET System. Calibration is an automated procedure that usually takes less than a minute to complete.

Prior to leaving the [Lifestyle Panel](#), do not forget to click the [Save](#) button to store the information from this page into the Client's [Previous Visits](#) history shown above.

At this time you may return to the [Demographic Profile](#), only if you forgot to add something to that screen. Make your changes, be sure to click save, and then return again to the Lifestyle Profile.

It is **RECOMMENDED** that you proceed to the optional panel called the [History Profile](#), particularly for first time clients. The [History Profile](#) provides a further and more in-depth view of what the client may be experiencing.

Always go directly to the [Wellness Info](#) to begin working with your client. However, should you decide to do the Body Biofield Test instead, you may access it from the [Wellness Info Panel](#).

Summary of Features:

- Interview client and place a number from 1 to 10 in each box
- Complete Calibration
- Option: Return to “Demographic Profile,” only if necessary, to make any changes
- Option: Go to “History Profile” (this is the next recommended step)
- Click “Save” to store information in Client’s Previous Visits history.
- Go directly to the “Wellness Info” panel.
- Should you desire to use the “Biofield Test” directly, click on that button from “Wellness Info”.

History Profile:

- Tonsils
- Brain Part
- Adenoids
- Appendix
- Gall Bladder
- Spleen
- Thyroid
- Uterus
- Ovaries
- Kidney
- Lung
- Nerve Part
- Stomach Part
- Intestine
- Thymus
- Right Arm, Complete
- Right Arm Below Elbow
- Right Hand
- Part Of Right Hand
- Right Finger Or Fingers
- Right Shoulder
- Right Leg Complete
- Right Leg Below Knee
- Right Foot
- Part Of Right Foot
- Right Toe Or Toes
- Right Eye Or Vision
- Right Ear Or Hearing
- Facial Disfigurement
- Bone Removed
- Breast Or Lymph Part
- Left Arm Complete
- Left Arm Below Elbow
- Left Hand
- Part Of Left Hand
- Left Finger Or Fingers
- Left Shoulder
- Left Leg Complete
- Left Leg Below Knee
- Left Foot
- Part Of Left Foot
- Left Toe Or Toes
- Left Eye Or Vision
- Left Ear Or Hearing
- Spinal Part
- Pelvic Part
- Testicle

Toxic Exposures:

- Radiation Exposure
- Food Additives
- Beauty Salon Toxins
- Industrial Toxins
- Asbestos, Fiberglass
- Heavy Metals
- Herbicide, Insecticide
- Chlorine Or Fluorine
- Air, Water Pollution
- Infectious Diseases

Major Diseases:

- Vascular, Circulatory Disease, Arteries, Veins
- Infections Or History Of Infections
- Cancer, Tumors, Or Degenerative Disease
- Dietary Disorders Or Absorption Disorders
- Drug Or Alcohol Addiction, Toxic Exposure
- Congenital Or Inherited Birth Disorders
- Allergies, Or Tendency To Allergies
- Any Serious Trauma Or Injury In History
- Endocrine, Glandular Or Hormonal Disorders
- Mental Or Emotional Disorders In History
- Sensory: Eyes, Ears, Taste, Feeling Or Smell
- Sensitivity To Humidity, Heat, Cold, Etc.
- Cognitive Or Memory Disorders

Types Of Stress

Describe:

Please Give A Brief Description Of The Kind Of Stress: Work, Family, Relationship, Etc.

Medications:

- Pain Meds.
- Blood Pressure
- Blood Thinners
- Cholesterol
- Kidney
- Anti-Convulsant
- Anti-Depressants
- Anti-Psychotic
- Cancer Drugs
- Antibiotics
- Steroids
- Liver
- Heart Medication
- Thyroid
- Digestive
- Diabetic Meds.
- Birth Control
- Parkinson's

Demographics

Inherited Disorders:

Mother:

Father:

Save

Lifestyle Profile

About Panel

History Profile

The [History Profile](#) contains six panels. Each panel displays generic information that may or may not pertain to your client. Check the appropriate boxes and/or enter text where indicated. Click the [Save](#) button prior to closing and all information will automatically be stored within the [Demographic Profile](#) history for future reference. When you have finished, click the [Lifestyle Profile](#) button at the lower right portion of the screen and you will be returned to that panel.

Summary of Features:

- Check any appropriate boxes in “History Profile”
- Check any appropriate boxes in “Toxic Exposures”
- Check any appropriate boxes in “Major Diseases”
- Check any appropriate boxes in “Medications”
- Describe any appropriate boxes in “Types of Stress”
- List any “Inherited Disorders”
- Click the “Save” button prior to closing, to store information in Demographics
- Click “Lifestyle Profile” button to return to that panel. Proceed to Reactivity Test.

ID	Item Name	Sgnif
3441	NITRO CUM ACIDUM	1302
4146	ST32 Fulu	1369
4549	Fungus E2	1342
5319	Dipyridum carinum	1337
5773	Sjilinal carifid	1310
1177	Hobowen Ashraling Sys	1306
4473	Debility	1368
6000	PCP #1	1361
5351	Pititralis	1353
4395	On leiniss carifid	1312
2540	Bulkus ninnate	1264
6016	Toxoplasma goncii	1775
2401	Selmonella Typhimurum	1750
1318	Argaroo 75	1742
1312	Campe, RY Wine	1727
1540	Super Dent nask, Alov	1718
6044	NPP MIX U5	1351
3577	STRAMONIL M	1374
3567	SPIRAN T-ES AUTUMNALS	1358

Indication Nitric Acid Selects for its special test of action the outlets of the body where the mucous membrane and skin meet; these pain as from splinters. Sticking pains. Marked improvement of all symptoms while riding in a carriage. Acts best on the dark complexioned and past middle life. Symplic, after abuse of Mercury. Faint appear and disappear quickly. Ball. Hydrogenoid constitution. Spleetic nature by Meters and woods in mouth, tongue, genital; blood poorly. Expires with pain during stool, as if rectum were torn. All discharges very offensive, especially urine, feces, and perspiration. Persons who have chronic diseases, and take cold easily and disposed to

Test Potential 1 Second Auto Feedback 10 Seconds

Previous Visits

- 3/25/2008 11:40:40 A
- 3/25/2008 12:14:18 P
- 3/20/2008 2:05:07 P

Set Time Metaspace Harness 96 Rectified

Navigation Page Personal Affirmation

Hour Panel Patient Name steile, beinaid

Body-Biofield Reactivity Test Profile

The [Body-Biofield Reactivity Test Profile](#) is considered one of the most important aspects of the I.M.A.E.T. System and contains a multiplicity of functions. The primary function is to obtain an informational biofeedback stress response.

Ask the client to relax and remain quiet and still while reactivity test is being performed. Start by clicking the red [Test Potential](#) button to initiate the automated reactivity process. The test will take between four and seven minutes to complete, during which time, the client's response to thousands of substances will be assessed. Click [Save](#) upon completion to store the test. To view a previously stored test, just click on a date in the [Previous Visits](#) box and then click the brown [Restore](#) button.

Each item in the matrix will produce a graphic, referred to as a "Fractal Image." The fractal represents the energetic signature of that substance in graphic form. Fractals are powerful representations of the energetic pattern.

The information provided, in the form of numerical percentages, bar graphs and subsequent descriptors, provides clues to those areas which produced a stress response and may require relaxation management. Since Biofeedback or Stress Management technicians **DO NOT** use this instrument to diagnose, treat or prescribe for disease, the information should be evaluated carefully and does not in any way represent the presence of any mental or physical illness.

The reactivity response ONLY takes into consideration the possibility of susceptibility, weakness, exposure, or pre-disposition to a certain stress factor or wellness inhibitor associated with the indicated item. **PLEASE REMEMBER:** only duly qualified and licensed health care practitioners may make assumptions relative to specific disorders or medical conditions.

Following the reactivity test, you have several options. You may highlight any item in the test matrix and click the button entitled [5 Second Auto](#) or click the button entitled [Feedback-30 Seconds](#). You may also set the timer, for a more lengthy feedback process.

To obtain more precise information regarding a single entry, highlight any item in the matrix and click the button called [Check Single Item](#). A numerical percentage will appear in the box next to the button. A response above 75% may be considered significant, as it is desirable to have a response potential of 75% or below for this specific test.

At the top right of the screen are 39 (or more) color-coded category buttons. Each of these buttons represents a specific group test of items. Click any one of these “[Category](#)” buttons to review the items within that category and the related reactivity value that was generated during the test process. You may use either the button entitled [5 Second Auto](#) or [Feedback-30 Seconds](#) to provide feedback to any category item. **Please Note:** Clicking the [ALL](#) button, located at the lower right corner of the category tabs group, will return the screen to the main test matrix.

If you wish to [create a PERSONAL item](#) matrix for future assessment and feedback purposes, you may do so by typing the name of the desired item into the [Item Name](#) field, then placing the desired item onto the test tray, located on the top of the interface box, then clicking the [Import](#) button. The item will automatically be imported into your [PERSONAL](#) database, assigned an energetic signature, and included in the [PERSONAL](#) matrix. You may also [Export](#), [Sort](#) or [Clear](#) any of the items entered. These items will be stored as a part of your [PERSONAL](#) matrix. They will not be included in the main matrix. You may run a test on your [PERSONAL](#) items by clicking the red [TEST](#) button.

Notice the timer at the bottom right portion of the screen. You will find this feature on every panel throughout the I.M.A.E.T. System. The default setting on the timer is always 3-minutes. You may use the scroll feature to select any amount of time, up to 30 minutes. Located on the timer graphic you will find two red buttons, which allow for switching from [Harness](#) to [Metaspace](#) mode. **If you select “0” on the timer while in Metaspace mode, you will override the timing mechanism and the system will continue to run until you click the Stop Feedback button. This feature is available throughout the entire program.** As you continue through the program, you will notice that each screen has a [Stop Feedback](#) feature. **Please Note:** Any time the [Metaspace](#) mode is selected on the timer, throughout the entire program, the lights will **NOT** be activated on the box.

The [% Rectified](#) field on the timer displays the approximate energetic response of the client, relative to the feedback process. A score of 85% or above is satisfactory.


One final feature is the highly useful [Search](#) function. Type the name of any item or condition into the field provided, click the search button, and all the items in the matrix containing information regarding your item, will appear in the window. Scroll these items to evaluate and make any selection you wish. Apply feedback if applicable. Click the [Clear](#) button before making another entry.

Reminder: You may interrupt feedback at any time by clicking the [Stop Feedback](#) button. You may also return to the main Wellness Info at any time by clicking the [Wellness Info](#) button.

Summary of Features:

- Click [Test Potential](#) and wait for test to be completed. Click Save-Yes, when complete to store the test
- To view a previously stored test click on date in Previous Visits, then Restore
- Select an item and Click “Apply Feedback 5 sec” or “Apply Feedback 3 min”
- Option: Click any category button at the top right, make a selection from the matrix and apply feedback for 5 sec., 30 sec., or set timer, if appropriate.
- Add items to Personal Matrix by typing in “Enter Item Name”, then “Start Import”
- Notice ability to switch from Harness to Metaspace on timer
- Notice ability to change timing for feedback
- Notice “Stop Feedback”
- Use “% Rectification field” to determine effect of feedback, using 85% or above as satisfactory
- Click the “Save” button prior to closing to store test
- Clicking the “All” button returns to the main test matrix after using category tabs
- Click “Wellness Info.”

Chiropractic Panel

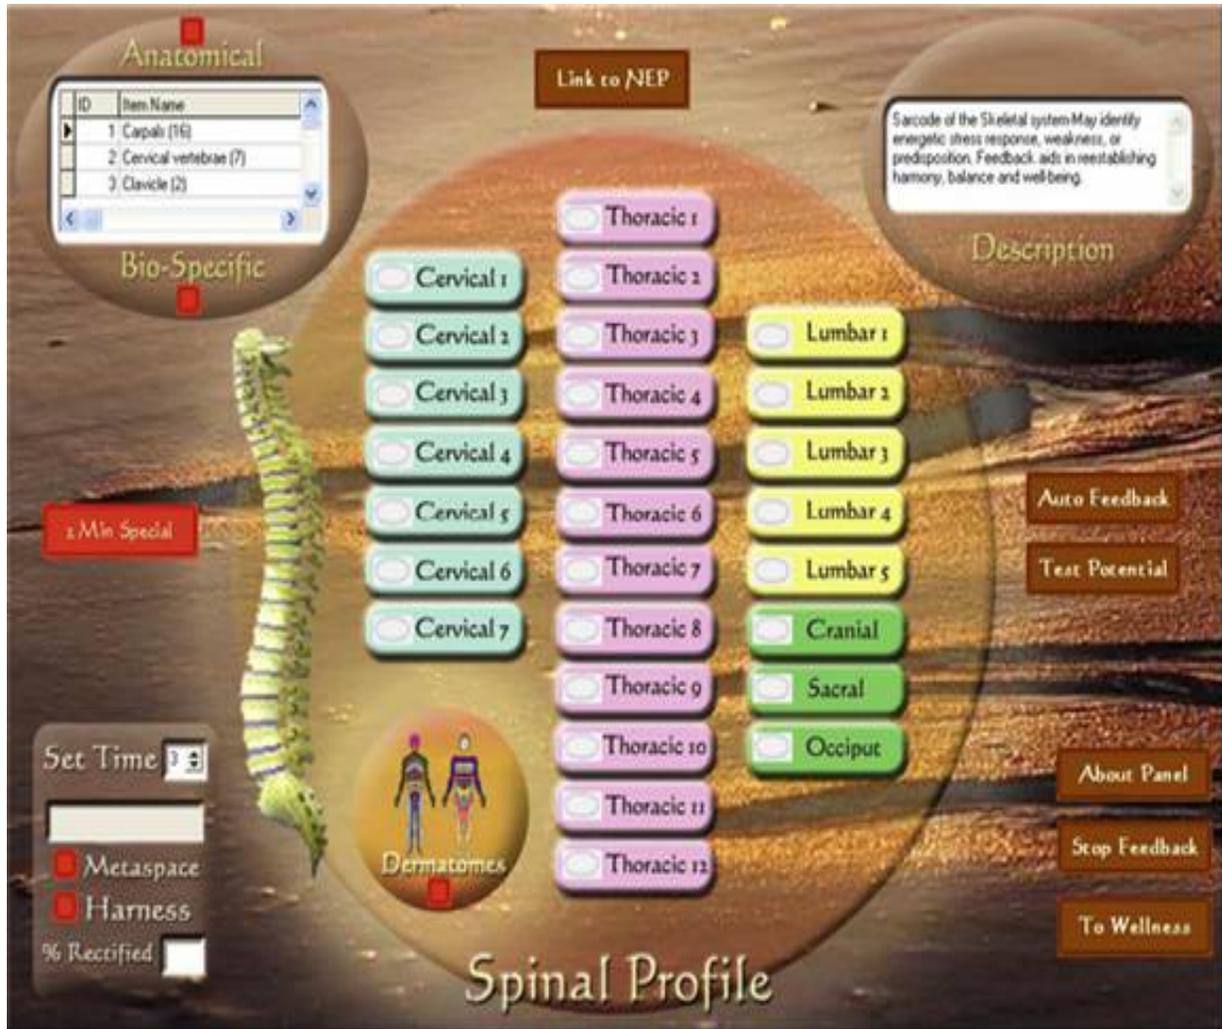

Spinal & Dermatome Profile

This panel provides insight into the energetic integrity of the spine. Select the [Test Potential](#) button to begin the reactivity process. Three colored markers will appear next to the vertebrae denoting the client's highest responses, with red as highest, then yellow and finally blue. Click the [Auto Feedback](#) button to begin the automated feedback procedure to the highest or red item ONLY. To initiate the feedback process to the top three items, set the timer to the desired length, click either the red [Metaspace](#) or [Harness](#) button to start, and the program will automatically divide the time allotted and apply feedback to each of the three items in succession. Continue with feedback until rectification reaches 85% or more. (The number of repetitions will vary with each individual).

Feedback may be applied to any *individual* vertebra by clicking on that vertebra, setting the time or using the three-minute default, and selecting either the [Metaspace](#) or [Harness](#) mode to start feedback. Again, desired rectification is 85% or more. Clicking [Stop Feedback](#) will interrupt feedback process.

You may access the [Neural-emotional Program \(N.E.P.\)](#) from this panel by clicking that button at the top center of the panel. After clicking the [Test Potential](#) button in the [NEP Profile](#), you may return to the [Spinal Profile](#) in order to view the influence the client's emotions have upon the spine.

To open and view the dermatome panel, click the red button next to [Dermatomes](#).


This will open a panel showing specific areas of the skin that provide sensory input via spinal nerves or the 5th Cranial Nerve. To apply feedback to any of these Dermatomes, set the timer, click the colored button representing that area of choice, then select either the red [Harness](#) or [Metaspace](#) button to activate the process.

By clicking on either the red [Anatomical](#) or [Bio-Specific](#) button at the top left of the page, a list or table of items will appear. You may select and highlight any one of these items and apply feedback by utilizing the timer in the standard manner. The item selected will have information provided in the Description field, offering a further understanding of the client's energetic profile.

When all balancing is complete, return to the [Spinal](#) panel or the [Wellness Info](#).

Summary of Features:

- Click "Test Potential" to gain a reactivity reading of the spine
- Select "Auto Feedback"
- Begin balancing of single items by setting timer
- Continue until rectification reaches 85% or more
- Option: Select a "Dermatome" for balancing, set timer and apply feedback
- Option: Use "Stop Feedback" at any time
- Option: Go to "Link to N.E.P."
- Option: Discover a primary "Anatomical" concern and select feedback
- Option: Discover a primary "Bio-Specific" concern and select feedback
- Option: Click on "2 Min Special" for visualization stimulation on healthy organ.

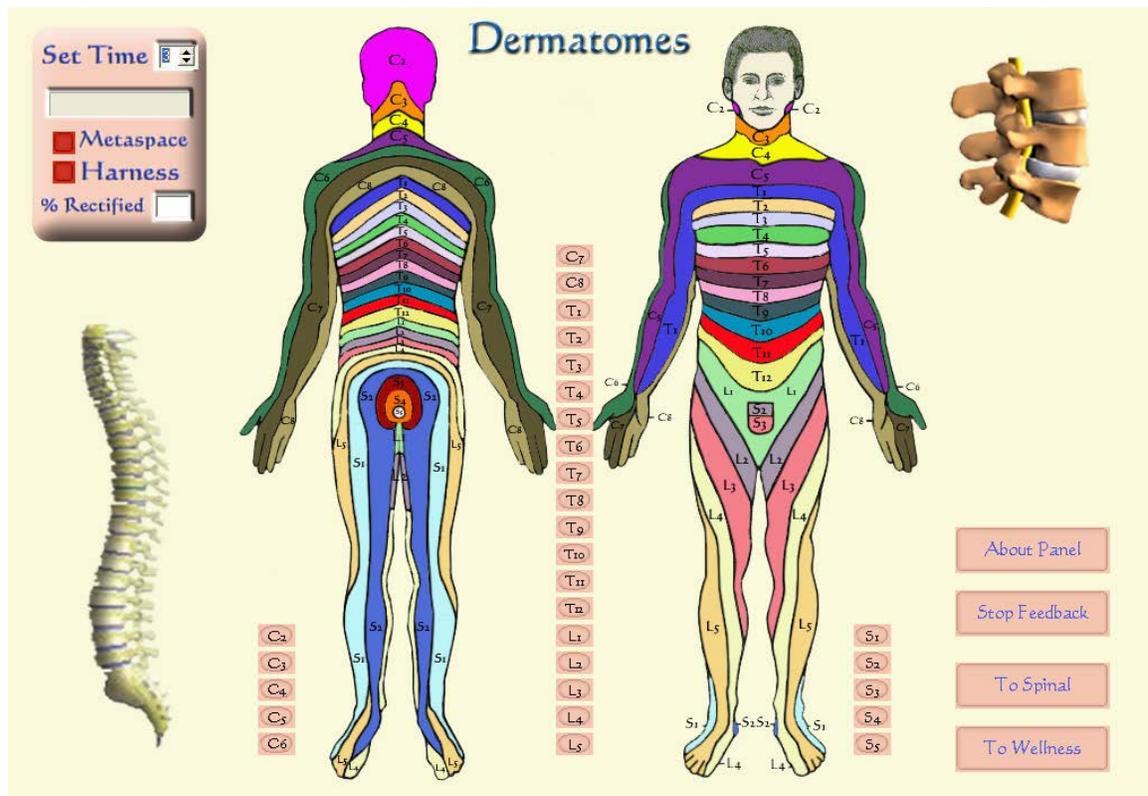



Neuro-Emotional Profile (N.E.P.)

This panel provided a sub-conscious link to a number of core emotional issues. To begin the evaluation process, click the [Test Potential](#) button. Upon completion, color values of red, yellow and blue will be displayed next to the three most reactive items. To initiate the feedback process to the top three items, set the timer to the desired length, click either the red [Metaspace](#) or [Harness](#) button to start, and the program will automatically divide the time allotted and apply feedback to each of the three items in succession. Otherwise the program will utilize the default time of 3 minutes.

If you wish to apply feedback to any specific item, select that item by clicking on it, adjusting the timer to the desired settings and then clicking either [Metaspace](#) or [Harness](#).

You may use the question fields at the top right of the screen to ascertain the client's involvement regarding certain issues.

Clicking the [Check Spinal Relationship](#) button will transfer you back to the [Spinal Profile](#) panel. The Spinal panel also provides a transfer button back to the [N.E.P. Profile](#) panel. Utilizing the Spinal panel at this time may help to determine where emotional issues are stored in the body. Simply click the [Test Potential](#) button in the Spinal panel, provide direction toward a possible solution then set the timer to the desired setting and click on either "[Harness](#)" or "[Metaspace](#)." Please remember that setting the timer to "0" and choosing "[Metaspace](#)", the program will run indefinitely until you select [Stop Feedback](#). This feature exists in all panels.

To use the [Unconscious Self-Evaluation Hint](#), click the red button provided at the left of the window. A hint, relative to the client's sub-conscious choice appears in the window, providing direction toward a possible solution. You may apply feedback for this issue by setting the timer in the standard manner.

When finished, simply return to the [Wellness Info](#) for subsequent choices.

Summary of Features:

- Click "Test Potential"
- Evaluate the top three findings
- Continue until rectification is 75% or above
- Option: Use the questions in the upper right section to assist in understanding the emotions you may wish to balance
- Option: Click "Check Spinal Relationship" to determine where the emotion may be blocking the flow of energy in the spine
- Set the timer or use the 3 minute default
- Select either the "Metaspace" or "Harness" mode
 - Option: You may Stop Feedback at any time
 - Option: Click the red button in the window under the "unconscious Self-Evaluation Hint" for finding information that may lead to a possible solution.
- When finished, Click on "Wellness Info"



Acupuncture – TCM Panel

This panel provides insight into the energetic integrity of the body's meridian system. Click the [Test Potential](#) button at the top center of the panel. The program will assess the relative stress potentials of the 14 basic meridian pathways. The three most reactive items will be indicated by color values, with red as highest, then yellow, and finally blue. To initiate the feedback process to the top three items, set the timer to the desired length, click either the red [Metaspace](#) or [Harness](#) button to start, and the program will automatically divide the time allotted and apply feedback to each of the three items in succession. Selecting the [Auto Feedback](#) button near the top center of the panel will activate an auto feedback process pertaining to the highest or red item ONLY.

Click any one of the six buttons next in the [Quadrant Feedback](#) panel to generate a feedback response for the selected quadrant. Set the timer for the desired duration and click either [Metaspace](#) or [Harness](#).

(Note that you may stop feedback at any time by clicking on the [Stop Feedback](#) button at the bottom left). Select [Reset](#) following the use of the Quadrant Feedback feature.

You may select any individual meridian group for feedback, other than the ones chosen by the computer, by clicking on the button next to the desired item. You may then set the timer in the standard manner to proceed with feedback.

A third option exists within the framework of this panel. An oval window, located at the bottom right of the screen contains all of the known Chinese acupuncture points. You may click on the [Test Potential](#) button to initiate a reactivity process relative to all the individual points in the table. Upon completion of the assessment process, three color values will be displayed denoting those items demonstrating the highest reactivity values. To initiate the feedback process to the top three items, set the timer to the desired length and the program will automatically divide the time allotted and apply feedback to each of the three items in succession. Set the timer then click either the [Metaspace](#) or [Harness](#) button to begin the feedback process.

In addition you may choose to apply feedback to any *single* point you wish, by clicking and highlighting the item, and then applying feedback by selecting the timer and pressing either “[Metaspace](#)” or “[Harness](#).” You will also notice that a detailed description of each point appears in the text window just below the graphic of Acu-Man.

Return to the [Wellness Info](#) to select another [Auto Program](#) or make another program selection.

Summary of Features:

- Click Test Potential to check integrity of the meridian system
- Select Auto Feedback to begin the energetic balancing
- Option: Select one of six quadrants for feedback. Select Reset upon completion
 - Select time
 - Option: Switch between Metaspace and Harness
 - Option: Stop Feedback any time desired
- Option: Select individual Chinese acupuncture point for feedback or choose Test Potential, set timer and apply feedback
 - Highlight desired acupuncture point
 - Select time
 - Option: Switch between Metaspace and Harness
 - Option: Stop feedback any time desired
- Return to Wellness Info

Chromosome Assessment

- All Chromosomes
- Auto Feedback 3 Min.

ID	Item Name
1	Chromosome 1-P
2	Chromosome 1-Q
3	Chromosome 10-P
4	Chromosome 10-Q
5	Chromosome 11-P

Chromosome & Gene Profile

Gene Assessment

- Select All Genes
- Auto Feedback 3 Min.

Disorder	Gene
1	Adrenoleukodystrophy
2	Alzheimer's disease

Adrenoleukodystrophy (ALD) is a rare, inherited metabolic disorder that afflicts the young boy Lorenzo Odone, whose story is told in the 1993 film "Lorenzo's oil." In this disease, the fatty covering (myelin sheath) on nerve fibers in the brain is lost, and the adrenal gland degenerates, leading to progressive neurological disability and death.

Cell-Com Profile

Auto Cell-com Tri-vector Feedback

Test Potential

ID	Item Name
1	Acid-base balance, support of
2	Acidophilus, normalization of
3	Addiction, treatment of (1)
4	Addiction, treatment of (2)
5	Addiction, treatment of (3)

3 Min. Auto Feedback

Set Time 3

Metaspace

Harness

% Rectified

About Panel

Stop Feedback

To Wellness

Chromosome, Gene & Cell-Com Profile

This panel combines a number of features including Chromosome and Gene feedback, as well as the use of Automated Cell-Com like programs.

For chromosome feedback, select either [All Chromosomes](#) then click the [Auto Feedback](#) button to initiate a 3-Minute feedback process. Or, choose [One Chromosome](#) by scrolling through the table, and then selecting the appropriate timer settings. If you wish to select a longer time, simply highlight an item in the list and use the default time of 3 minutes, or change the time, and click on either the [Metaspace](#) or the [Harness](#) button.

For gene feedback, select either [Select All Genes](#) then click the [Auto Feedback](#) button to initiate a 3-Minute feedback process. Or choose [Select One Chromosome](#) by scrolling through the table, highlighting an item and then selecting the appropriate timer settings. If you wish to select a longer time, simply highlight an item in the list and use the default time of 3 minutes, or change the time, and click on either the [Metaspace](#) or the [Harness](#) button.

By clicking the red [Start Feedback](#) button on the circular [Auto Cell-Com, Feedback](#) Panel the program will begin a reactivity process, which will suggest three feedback processes. Upon completion of the assessment process, three color values will be displayed denoting those items demonstrating the highest reactivity values. To initiate the feedback process to the top three items, set the timer to the desired length, click either the red [Metaspace](#) or [Harness](#) button to start, and the program will automatically divide the time allotted and apply feedback to each of the three items in succession. Click either the [Metaspace](#) or [Harness](#) button to begin the feedback process.

Upon clicking the red [3 Min. Auto Feedback](#) button the program will automatically administer a feedback process to the item highlighted in red. Or you may scroll through the table to make an individual selection of your choice. Simply highlight the chosen item, set the timer to the desired length and choose either [Metaspace](#) or [Harness](#) to deliver feedback.

As with all programs, you may use the [Stop Feedback](#) button at any time. When finished, click the [Wellness Info](#) button.

Summary of Features:

- Balance one or all chromosomes using “Auto Feedback” or setting timer
- Balance one or all genes using “Auto Feedback” or setting timer
- To use “Tri-Vector Cell-Com” feature, click “Auto Select & Feedback” button
 - Option: Change the default timer
 - Make an individual selection in any of the three tables
 - Option: Switch between “Metaspace” and “Harness”



Organ Specific Sarcodes

This panel provides feedback options for 43 different organs. They have been prepared using the Homeopathic signature of each organ represented in the matrix.

Click the button next to the organ or function you wish to address in either of the blue, green, red or purple panels. You may select and balance **ONLY ONE ORGAN AT A TIME**. However, you may check as many [Add Additional Feedback](#) items as you wish. They are located in the pale green oval at the top center of the panel.

To begin the feedback process, select the desired time or use the 3-minute default. The timer may be set to a maximum of 30 minutes in the Harness mode. While in the Metaspace mode the timer may be set to either a prescribed time or “0” for an unlimited duration. Click the [Stop Feedback](#) button to discontinue feedback.


Return to the [Wellness Info](#) for another choice.

Organ Specific Sarcodes

Summary of Features:

- Click on the desired organ
- Click on the “Add Additional Feedback”

- Set time or leave at the 3 minute default
 - Option: Discontinue by clicking the “Stop Feedback” bar
- Check either Metaspace or Harness mode

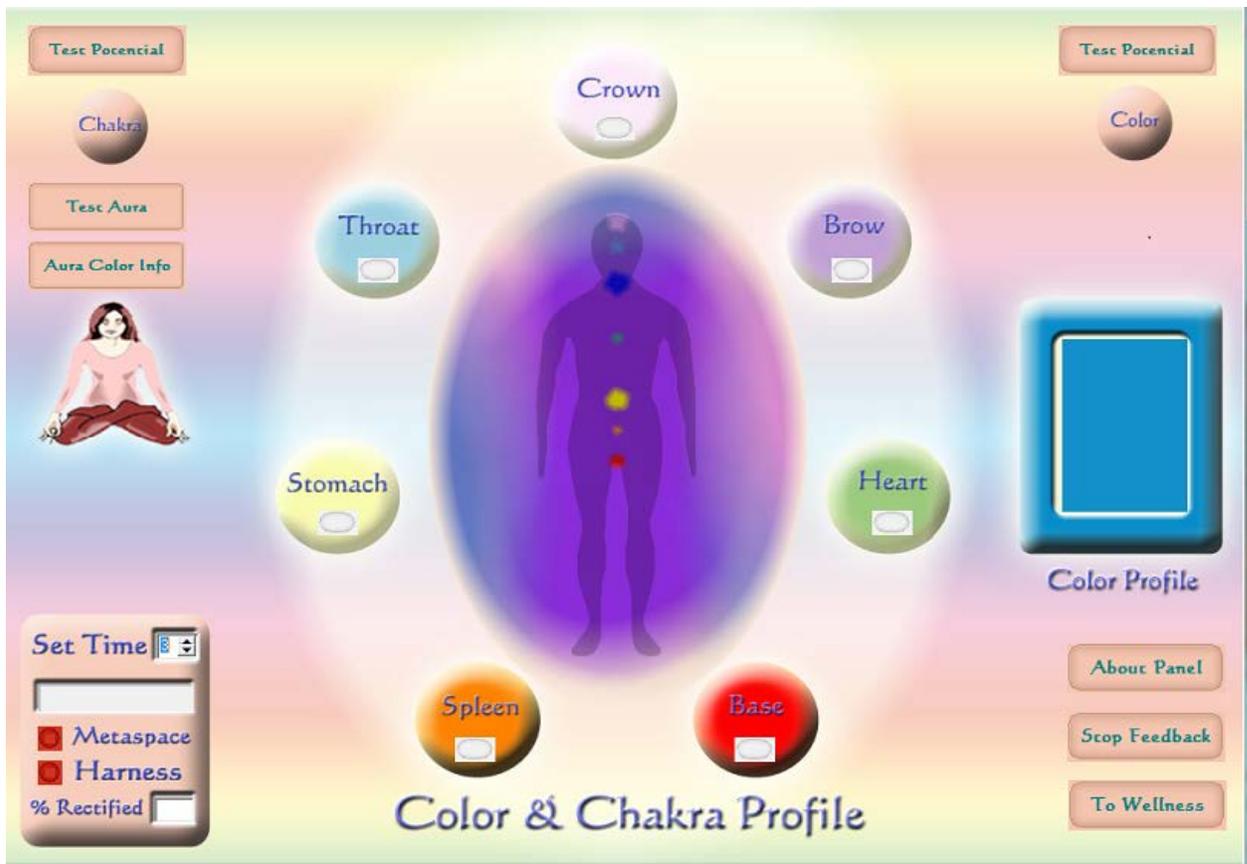

Color, Chakra & Aura Profile

As indicated by the title, there are three main functions performed from this panel. To use the [Color Profile](#) as a feedback modality, click the [Test Color](#) button located on bar at the top of the screen. Upon completion, the program will display, in the Color Profile box, the color most likely to have a profound feedback influence on the client. To give that color's feedback signature to the client, select the appropriate options on the timer, located at the lower left side of the page. You have the option to change the time or switch to [Harness](#) or [Metaspace](#). *Default settings are for 3 minutes.* The [% Rectified](#) window should be 85 or above. As a technician, you may drape the client in that color for the session, or recommend that the client wear that color for a period of time between appointments.

To run the [Chakra Profile](#), click the [Test Chakra](#) button located on the bar at the top of the screen. Upon completion, the program will display three, color values in the circular graphics surrounding the central chakra graphic. The top three values will be identified in red, yellow and blue respectively. To initiate the feedback process to the top three items, set the timer to the desired length, click either the red [Metaspace](#) or [Harness](#) button to start, and the program will automatically divide the time allotted and apply feedback to each of the three items in succession.

As with the color program, you may change the length of time and mode of delivery. If you wish to balance just one Chakra click on the white rectangular button within the specific charka, and adjust the timer as needed. The % Rectified window should be 85 or above for either method of balancing.

To start the [Aura Profile](#) simply click [Test Aura](#) button at the left of the screen. The test results will be displayed in approximately 1-1/2 minutes. To evaluate the meaning of the rendered colors and their position within the graphic, please read the brief descriptions provided by clicking the [Aura Color Info](#) button. For more in depth evaluation please read one of the many books that have been written on the subject of Aura interpretation. For each of the programs, you may interrupt feedback at any time by clicking the [Stop Feedback](#) button. Return to the main program screen when finished, by clicking the [Wellness Info](#) button.

Summary of Features:

Select one of the following:

For Color balancing

- Click “Test Color” button
- Review color presented in the Color Profile box
- To start color balancing, make appropriate selections on timer
 - Option: Change the default timer of 3 minutes
 - Option: Change mode of delivery

For Chakra balancing

- Click “Test Chakra” button
- Review red, yellow & blue reactivity indicators of the charkas in circles around the central charka image
- To start charka balancing of three top chakras, make selections on timer
- For any program you may use the “Stop Feedback” button
- Return to the “Wellness Info” screen when completed
 - Option: Balance a single charka by first clicking the rectangular button, then making appropriate selections on timer

For Aura balancing

- Click “Test Aura” button
- Review the “Aura Color Info” for interpretation
- Click “Wellness Info” button when finished

CARDIO - Panel

The Cardio Panel interface includes the following components:

- Circulatory System:** A 3D anatomical model of the heart.
- Transfer Functions:** A list of checkboxes for transferring energy to various body parts: Ears/Eyes, Muscles, Bones, Respiratory, Nerves, Lymph, Sinuses, and Digestive.
- Valves & Conduction:** A sub-panel with a "Set Time" input, checkboxes for "Metaspace" and "Harness", a "% Rectified" input, and checkboxes for "Test Potential" and "Chelation Stim.". It also features a table of heart valves and a descriptive text box.
- Circulatory Profile:** A section with a "2 Min Special" button, a "Select Bio-Specific" list (Aneurysm, Angina Pectoris, Phlebitis, Stroke), and an "Add Emphasis" list (Inflammation, Infection, Degeneration, Pain).
- Navigation:** Buttons for "About Panel", "Stop Feedback", and "To Wellness".
- Interactive Callout:** A circular callout titled "Click Item To Select View Function Above" showing a table of heart components and checkboxes for "Bio-Specific Stress" and "Anatomical".

ID	Item Name
1	Aortic Valve
2	Atrioventricular Node-AV
3	Left Atrium

The Aortic valve opens the way for oxygen-rich blood to pass from the left ventricle into the aorta, your body's largest artery, where it is delivered to the rest of your body.

ID	Item Name
1	Aortic Valve
2	Atrioventricular Node-AV
3	Left Atrium
4	Left Ventricle
5	Mitral Valve
6	Pulmonary Valve

The functions associated with this page are similar to nine other panels that include Muscles, Cartilage & Ligaments, Respiratory, Digestive, Sinuses, Nerves, Lymph, Ears & Eyes, Dental and Bone Profiles.

Each panel contains two feedback procedures with the Exception of the Circulatory & Heart Profile and the Muscles, Cartilage & Ligaments Profile.

Two features are located in the rectangular panel at the lower left of the screen. The left portion of the panel contains four of the *most commonly occurring* Bio-Specific items associated with Circulatory & Heart Profile. Click on one or all of the items under Select Bio Specific items. The right portion of the rectangular panel contains items that Add Emphasis to the balancing and feedback process. You may select one or all items for emphasis. To initiate feedback, select the time or use the 3-Minute default, and click on either the Metaspace or Harness button to start.

In the lower right corner of the [Circulatory & Heart Profile](#) panel is an oval graphic that contains a scrollable list of [Bio-Specific](#) and [Anatomical](#) items. Click the red [Bio-Specific Stress](#) button to find an expanded list of conditions that are specific to the [Circulatory & Heart Profile](#). Click the red [Anatomical](#) button to switch to an expanded list of anatomical parts associated with the [Circulatory & Heart Profile](#). You may apply feedback to any item you select, in either of the lists by highlighting the item desired, setting the timer to the desired length (unless you use the 3-minute default setting) then clicking either the red [Metaspace](#) or [Harness](#) button to enable the feedback process. Upon choosing any item in the Bio-Specific Stress or anatomical List, an educational description of that item appears in the text box directly above.

In the upper right of this panel, you see an additional feature called [Valves & Conduction](#). Click the red [Test Potential](#) button to initiate a reactivity test that will provide a status assessment, showing the top three items highlighted in red, yellow and blue. To initiate the feedback process to the top three items, set the timer to the desired length and the program will automatically divide the time allotted and apply feedback to each of the three items in succession. Or you may choose to apply feedback to a single item by highlighting the chosen valve, set the timer (or use the 3-minute default), and clicking on [Metaspace](#) or [Harness](#) to start the procedure. You may stop feedback at anytime by clicking the [Stop Feedback](#) button.

In addition to features mentioned, you will see that eight transfer buttons are located in the upper central portion of the screen. Clicking a [Transfer](#) button enables quick access to a different panel without the necessity of returning to the [Wellness Info](#).

Summary of Features:

- Click “Select Bio-specific” items from the rectangle box on the lower left
- Click “Add Emphasis” items from the rectangle box on the lower left
- To begin feedback, select time (or use the 3 minute default) and click “Metaspace” or “Harness” to start the feedback
- For an expanded view of functions go to the oval image in the lower right
 - Click “Bio Specific Stress” or “Anatomical”
 - Highlight a single item and read about it in the dialog box above
 - To begin feedback with single items, select time (or use the 3 minute default) and click “Metaspace” or “Harness” to start the feedback
- Stop feedback at any time by clicking “Stop Feedback”
- Go to the box in the upper right and click on Valves & conduction.
- Click on Test Potential to obtain a reactivity assessment
 - To begin feedback with single items, select time (or use the 3 minute default) and click “Metaspace” or “Harness” to start the feedback
- Option: Use transfer buttons to go to other programs in this grouping
- Option: Click on “2 Min Special” for visualization stimulation on healthy organ.
- Option: Return to the “Wellness Info”

Lymph System

Lymph Profile

2 Min Special

Set Time: 3

Metaspace
Harness
% Rectified

Transfer To Circulation
Transfer To Muscles
Transfer To Respiratory
Transfer To Digestive
Transfer To Nerves
Transfer To Bones
Transfer To Ears/Eyes
Transfer To Sinuses

Click Item To Select View Function Above

ID	Item Name
1	accessory nodes
2	anterior auricular nodes
3	anterior jugular nodes
4	anterior mediastinal nodes
5	apical axillary nodes
6	auricular nodes, anterior

Bio-Specific Stress
Anatomical

About Panel Stop Feedback To Wellness

Lymph Profile

The functions associated with this page are similar to nine other panels that include Muscles, Cartilage & Ligaments, the Circulatory, Respiratory, Digestive, Nerve, Bone, Sinus, and Ears & Eyes Profiles.

Each panel contains two feedback procedures with the Exception of the Circulatory & Heart Profile and the Muscles, Cartilage & Ligaments Profile.


Two features are located in the rectangular panel at the lower left of the screen. The left portion of the panel contains four of the *most commonly occurring* **Bio-Specific** conditions associated with the **Lymph Profile**. Click on one or all of the items under **Select Bio Specific** items. The right portion of the rectangular panel contains items that **Add Emphasis** to the balancing and feedback process. You may select one or all items for emphasis. To begin feedback, select the time or use the 3-minute default, and click on either the **Metaspace** or **Harness** button to start. You may stop feedback at anytime by clicking the **Stop Feedback** button.

In the lower right corner of the [Lymph Profile](#) is an oval graphic that contains a scrollable list of [Bio-Specific](#) and [Anatomical](#) items. Click the red [Bio-Specific Stress](#) button to find an expanded list of conditions that are specific to the [Lymph Profile](#). Click the red [Anatomical](#) button to switch to an expanded list of anatomical parts associated with the [Lymph Profile](#). You may apply feedback to any item you select, in either of the lists by highlighting the item desired, setting the timer to the desired length (unless you use the 3-minute default setting) then clicking either the red [Metaspace](#) or [Harness](#) button to enable the feedback process. Upon choosing any item in the Bio-Specific Stress or Anatomical list, an educational description of that item appears in the text box directly above.

In addition to features mentioned, you will see that eight transfer buttons are located in the upper central portion of the screen. Clicking a [Transfer](#) button enables quick access to a different panel without the necessity of returning the [Wellness Info](#).

Summary of Features:

- Click “Select Bio-specific” items from the rectangle box on the lower left
- Click “Add Emphasis” items from the rectangle box on the lower left
- To begin feedback, select time (or use the 3 minute default) and click “Metaspace” or “Harness” to start the feedback
- For an expanded view of functions go the oval image in the lower right
 - Click “Bio Specific Stress” or “Anatomical”
 - Highlight a single item and read about it in the dialog box above
 - To begin feedback with single items, select time (or use the 3 minute default) and click “Metaspace” or “Harness” to start the feedback
- Option: Stop feedback at any time by clicking “Stop Feedback”
- Option: Use transfer buttons to go to other programs in this grouping
- Option: Click on “2 Min Special” for visualization stimulation on healthy organ.
- Option: Return to the “Wellness Info”

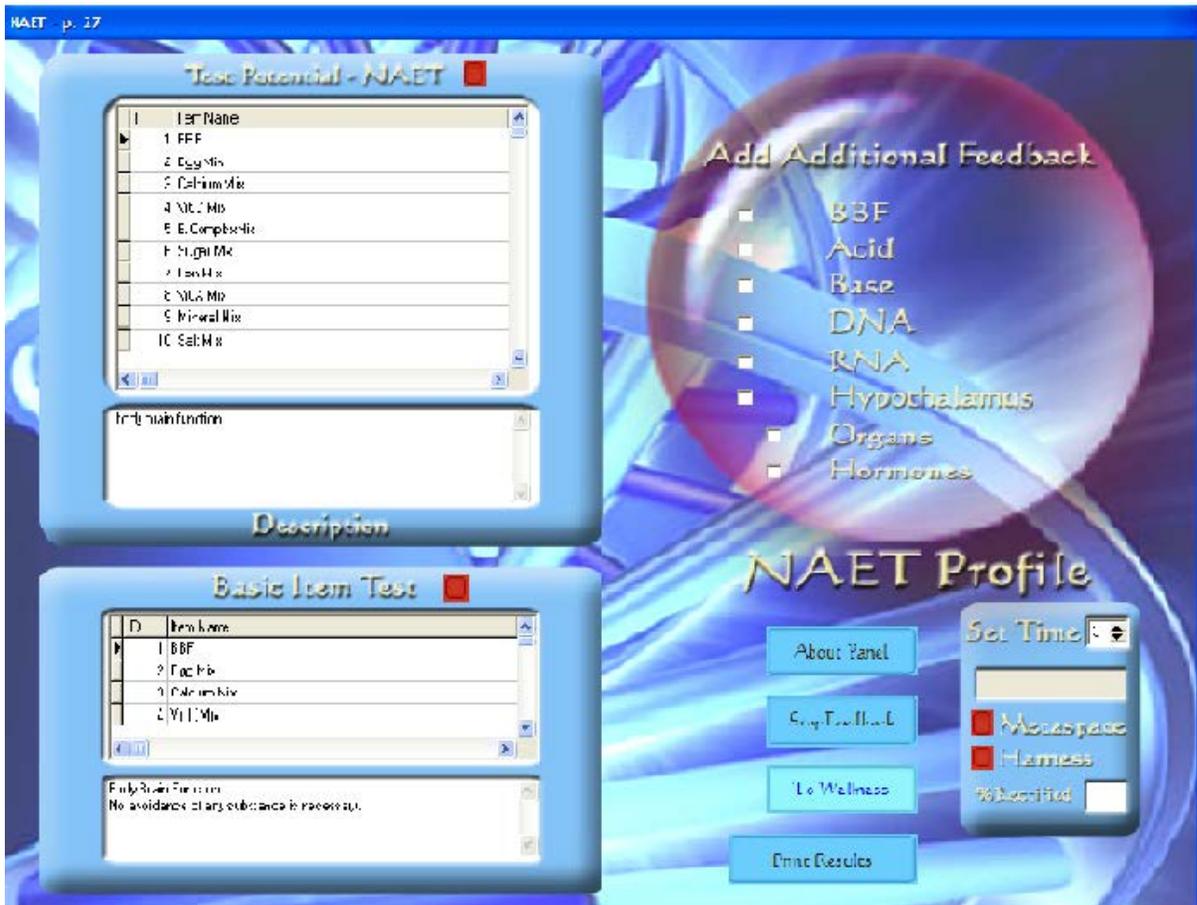

NAET Profile Panel

The **NAET Profile** screen contains several important features. The upper left corner of the screen provides a view of the NAET program reactivity items. 23 test kits plus misc. items or 1801 pre-programmed items appear in this scrollable list. Click on the red **Test Potential-Comprehensive Database** button to perform a reactivity test. The *three highest reactivity values* will be displayed along with their numerical values and highlighted in red, yellow and blue respectively. To apply feedback, select the red **Metaspace** or **Harness** button to perform an automatic 1-minute quick feedback procedure of each of the top 3 items. For a longer feedback procedure, set the timer to the desired feedback length (or leave the 3-minute default setting) and then click **Harness** or **Metaspace** to initiate feedback. To stop feedback, click the **Stop Feedback** button. If you desire to feedback a single item, click on that item and then click on **Metaspace** or **Harness** to initiate feedback.

In the upper right is a circular graphic containing additional feedback items. Place a check in *any or all of the boxes* found in the **Add Additional Feedback** panel. Then click the red **Metaspace** or **Harness** button in the rectangular box on the right to perform an automatic 1-minute quick feedback procedure. For a longer feedback procedure set the timer to the feedback length (or leave the 3-minute default setting) and then click **Harness** or **Metaspace** to initiate feedback. To stop feedback, click the **Stop Feedback** button.

If you use the default setting for feedback, the **additional feedback** items will be automatically added at the end of the main feedback at a 1/6 time interval. i.e. a 3 minute feedback will be divided into 1 minute each for the top 3 main reactivity items and 10 seconds for each selected **additional feedback** item.

The lower left corner provides a view of the [Basic Items Test](#). The first 3 NAET kits, 234 pre-programmed basic items appear in this scrollable list. Click on the red [Basic Items Test](#) button to perform a reactivity test. The three highest reactivity values will be displayed and highlighted in red, yellow and blue respectively. To apply feedback, follow the same procedures as with the [Comprehensive Database](#) NAET test.

The [Print Results](#) button will allow you to view and save a printable version of your top ten test results. It will save it in a document folder for later retrieval or e-mail attachment. To retrieve saved results go to: my documents – click on ImaetSys folder – click on patient reports – click on individual patient’s folder – and finally click on the selected testing or assessment date.

Please note: Feedback choices and selections can only be saved in the multiple item “Custom Treatment Data” field. To record single treatments off the regular NAET Profile page, you still must maintain a patient chart!

Return to the main menu by clicking the [Wellness Info](#) button.

Summary Of Features:

The NAET Profile

- Click on the red “Test Potential-All” items to perform a reactivity test of all 1560 NAET items.
- To apply 1- minute feedback on each of the top 3 items, click the red “Metaspace” or “Harness” button.
 - Option: For longer feedback set the timer to the desired feedback length (or leave the 3-minute default setting)
 - Option: Click Harness or Metaspace to initiate feedback.
 - Option: To stop feedback, click the Stop Feedback button.

Add Additional Feedback

- Place a check in *any or all of the boxes* found in the “Add Additional Feedback panel.”
- To perform a 3-minute feedback procedure, click the red “Metaspace” or “Harness” button
 - Option: For a longer feedback procedure set the timer to the desired feedback length (or leave the 3-minute default setting)
 - Option: Click “Harness” or “Metaspace” to initiate feedback.
 - Option: To stop feedback, click the Stop Feedback button.

The Basic Items Test

- Click on the red “Test Potential-Basic Items Test” to perform a reactivity test of the first 3 NAET kits items.
- To apply 3- minute feedback on select a single item, click the red “Metaspace” or “Harness” button.
 - Option: For longer feedback set the timer to the desired feedback length (or leave the 3-minute default setting)
 - Option: Click Harness or Metaspace to initiate feedback.
 - Option: To stop feedback, click the Stop Feedback button.

PLEASE NOTE: You may only do one test panel per visit!! Either the Basic Items Scan (first 3 kits), or the full NAET Potential Scan (all 23 kits).


Follow up on your result with a NAET treatment or IMAET feedback!

Combination Treatment Basket:

The screenshot displays the NAET software interface. On the left, the 'Source Data' panel lists various items for selection, including Endorphin, Enkephalin, Heparin, Heat Labile Proteins, Histamines, Interferones, Interleukins, and Interleukin-1 through Interleukin-10. On the right, the 'Custom Treatment Data' panel shows a table with 6 items selected and highlighted in yellow: 1 Salmonella Typhi, BAC 78; 2 Salmonella Spp., BAC 77; 3 Salmonella typhi, BAC 79; 4 Shigella dysenteria, BAC 80; 5 Interleukin-5; and 6 Heat Labile Proteins. Below the panels, there are control buttons: 'Add >', '<Rem', '<<Rem All', and 'Clr Feedback'. An 'Additional Feedback' section includes checkboxes for BBF, Acid, Base (checked), DNA (checked), RNA, Hypothalamus (checked), Organs (checked), and Hormones. At the bottom, the 'Client' field contains 'straille, bernard', and the 'Previous Visits' table shows three entries with dates and times. A 'Set Time' dropdown is set to '3', and a '% Rectified' field is empty. Buttons for 'Close', 'Stop Feedback', 'Harness', and 'Save' are also visible.

The “Comprehensive Database” reactivity test results allow for a custom treatment ‘basket’ to pop up, by right clicking within that field. Then just add the combinations you want to be part of your feedback by highlighting the item in the left column and clicking add. This will move it into the right custom data treatment basket.

Here you can save your feedback information below under ‘previous visits’ by clicking “save”.

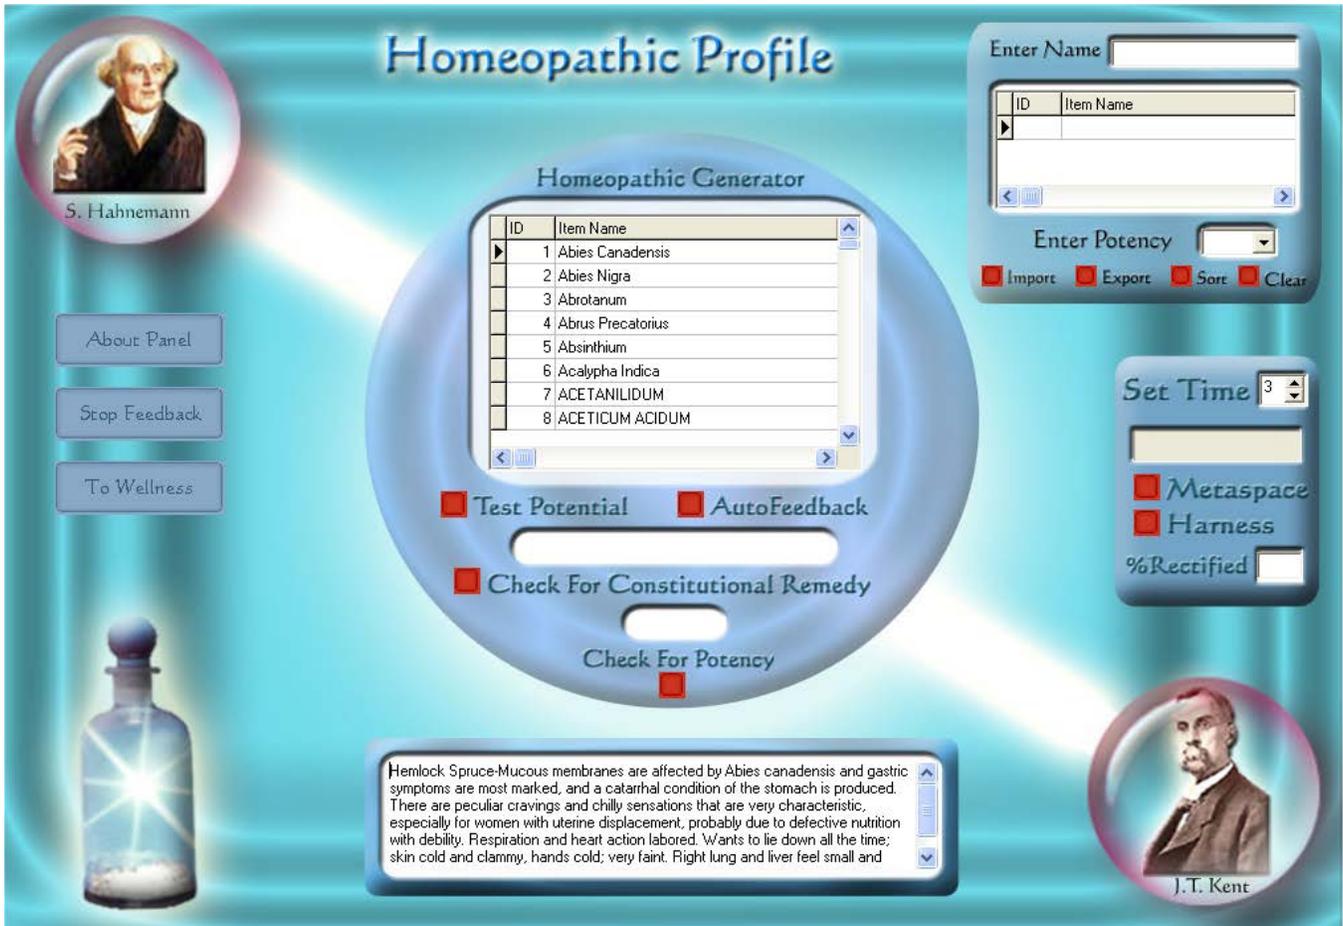

Homeopathic Profile

Homeopathic Reactivity Test And Feedback Procedure

In the upper central portion of the screen is a circular graphic containing a scrollable list of all pre-programmed Homeopathic remedies from A to Z. *To test a single item*, click the red **Test Potential** button below the list to initiate a reactivity test. The *three highest reactivity* values will be displayed and highlighted in red, yellow and blue respectively. To initiate the feedback process to the top three items, set the timer to the desired length, click either the red **Metaspacer** or **Harness** button to start, and the program will automatically divide the time allotted and apply feedback to each of the three items in succession. If you click the red **Auto Feedback** button you will initiate feedback to the red item ONLY. Or, you may also select any INDIVIDUAL item by highlighting it, then set the timer to the desired feedback length (or leave the 3-minute default setting), and click either the **Harness** or **Metaspacer** button to initiate feedback. The **% Rectified** results are displayed in the timer. An 85% or greater rectification is satisfactory. You may repeat the process up to 3 times in a single session, to achieve the desired result. If the desired result is not achieved, schedule an additional appointment within one week. You may also stop feedback by clicking the **Stop Feedback** button.

Check Constitutional Remedy

Click the red [Check for Constitutional Remedy](#) button. A suggested remedy will appear in the white field. To check for potency, click the red [Check for Potency](#) button. A result

will appear in the white field. To apply feedback, click the red [1-Min Feedback](#) button. You have the option of offering longer feedback by setting the timer (or leave the 3-minute default setting), then clicking either the [Harness](#) or [Metaspace](#) button to initiate feedback.

Exporting A Remedy To The Tray From Personal Database List

Near the top right of the screen, type in the name of any remedy in the white field next to the [Item Name](#) and import it into the data base list. Be sure to type the name exactly as you wish it to be stored in your personal database. Enter a potency, from the drop-down list into the [Enter Potency](#) field. Highlight the item in the list that you want to export, then click the red [Export](#) button. That signature will energetically charge the water or alcohol medium you have placed on the tray.

Importing A Remedy From The Tray To Personal Database List

Enter the name of the remedy you have placed on the tray in the [Item Name](#) field provided near the top right of the screen. Enter a potency, from the drop-down list into the [Enter Potency](#) field. Click the red [Import](#) button to activate the procedure. The item you entered will automatically appear in your personal database list.

When you have completed this program return to the main Wellness Info by clicking the [Wellness Info](#) button.

Summary of Features:

Homeopathic Reactivity Test

- *To test a single item*, click the red “Test Potential” button near the top of the green rectangle.
- Select an item by highlighting it, and then click the red “Auto Feedback” button to perform a brief automatic 1-minute quick feedback procedure.
- Option: For longer feedback, set the timer to the desired feedback length (or leave the 3-minute default setting)
- Option: Click either the “Harness” or “Metaspace” button to initiate feedback.
- You may repeat the process up to 5 times in a single session
- You may also stop feedback by clicking the “Stop Feedback” button.

Check Constitutional Remedy

- Click the red “Check for Constitutional Remedy” button.
- To check for potency, click the red “Check for Potency” button.
- To apply feedback, click the red “1-Min Feedback”
 - Option: Select desired time(or leave the 3-minute default setting)
 - Option: Click either the “Harness” or “Metaspace” button to initiate feedback.

Exporting a Remedy to the Tray

- Type in the name of any remedy in the white field next to “Enter Name”
- Enter the potency in the “Enter Potency” field.
- Click the red “Export” button to charge the median on the tray.

Importing a Remedy from the Tray

- Enter the name of the remedy you have placed on the tray in the “Enter Name” field”

Click the red “Import” button to activate the procedure.



Nutritional Profile

Nutritional Reactivity Test

Click one of the three red **Test Potential** buttons located in the mid-left portion of the screen to begin a reactivity process for the group of nutrients selected: Vitamins, Minerals or Amino Acids. **YOU MAY TEST ONLY ONE GROUP AT A TIME.** When complete, the chosen group will display the three highest reactivity values in red, yellow and blue respectively. To initiate the feedback process to the top three items, set the timer to the desired length, click either the red **Metaspace** or **Harness** button to start, and the program will automatically divide the time allotted and apply feedback to each of the three items in succession. After completing the three reactivity tests you may proceed to click on any single item in the three panels. A description of that item will appear in the dialog box in the center of the page.

Applying Additional Feedback

You may apply feedback to any **SINGLE** item or nutrient you select in each of the three panels. Click the button next to the item chosen, set the timer, or use the 3-minute default, then click either the **Metaspace** or **Harness** button to begin feedback. You may stop feedback by clicking the **Stop Feedback** button.

Testing an Item on the Tray

Place a substance on the stainless steel plate on top of the interface box, then click the red [Test Tray Item](#) button located in the middle left of the screen. In the white box below the button you will see a numerical reactivity value on a scale from 1 to 100. A value above 75% indicates a significant need.

Testing an Organ for a Specific Nutrient Need

Type the name of an organ in the white field in the center of the screen. Then type the name of a nutrient in the [Nutrient](#) field. Click the red [Test Energetic Imbalance](#) button and a numerical percent of need between 1 and 100 will be provided in the [%](#) field box. A value above 75% indicates a significant need.

When finished, return to the main Wellness Info by clicking the [Wellness Info](#) button.

Summary of Features:

Nutritional Reactivity Test

- Click the red “Test Potential” button located in the mid-left portion of the screen.
- Each group will display the three highest reactivity values in red, yellow and blue respectively.
- Click on a single item in any of the three panels to read a description of that item
- Review the numerical reactivity value on the timer

Applying Feedback

- Click the button next to the item chosen, set the timer or use the 3-minute default
- Click either the “Metaspace” or “Harness” button to begin feedback.
 - Option: Stop feedback by clicking the “Stop Feedback” button.

Testing an Item on the Tray

- Place a substance on the stainless steel plate on top of the interface box
- Click the red “Test Tray Item” button located in the middle left of the screen.
- Review numerical reactivity value on the timer

Testing an Organ for a Specific Nutrient Need

- Type the name of an organ in the white “Organ” field in the center of the screen.
- Type the name of a nutrient in the Nutrient field.
- Click red “Test For Energetic Imbalance” button to review numerical reactivity value in the [%](#) field.

Individual Female or Male Selections: Use the rectangular pink [Female Hormone Balance](#) or the rectangular blue [Male Hormone Balance](#) panel to provide a quick

option for applying feedback *without the use of reactivity testing*. *Select one item at a time*. Click the red [1-minute Feedback](#) button to start the process. For longer feedback, set the time or use the 3-minute default, then click either the red [Metaspace](#) or [Harness](#) button to start. To interrupt feedback, click the Stop Feedback button.

Ovarian & Prostate Stimulation: The [Ovarian Stim](#) and [Prostate Stim](#) panels are provided on either side of the screen. Click the red button to initiate a 3-minute auto feedback.

You may return to the main program list by clicking the [Wellness Info](#) button at any time.

Summary of Features:

Reactivity Testing


- To initiate Reactivity Testing for a *female*, click the red button titled “Test Potential” located in the pink circular graphic
- To initiate Reactivity Testing for a *male* client, click the red button titled “Test Potential” located in the blue circular graphic
- To begin feedback, highlight a chosen item, set the timer or use the 3-minute default, then click either the red “Metaspace” or “Harness” button to start.
 - Option: To interrupt feedback, click the “Stop Feedback” button.

Balance Female or Male Hormones

- Balance Female or Male Hormones by clicking next to the desired hormone
- Click the red “1-minute Feedback” button to start the process
 - Option: Set the time or use the 3-minute default
 - Option: Click either the red “Metaspace” or “Harness” button to start.
 - Option: To interrupt feedback, click the “Stop Feedback” button.

Ovarian Stim or Prostate Stim

- For Ovarian Stim or Prostate Stim, Click the red “3 minute Auto” button.
 - Option: Set the time or use the 3-minute default
 - Option: Click either the red “Metaspace” or “Harness” button to start.
 - Option: To interrupt feedback, click the “Stop Feedback” button.

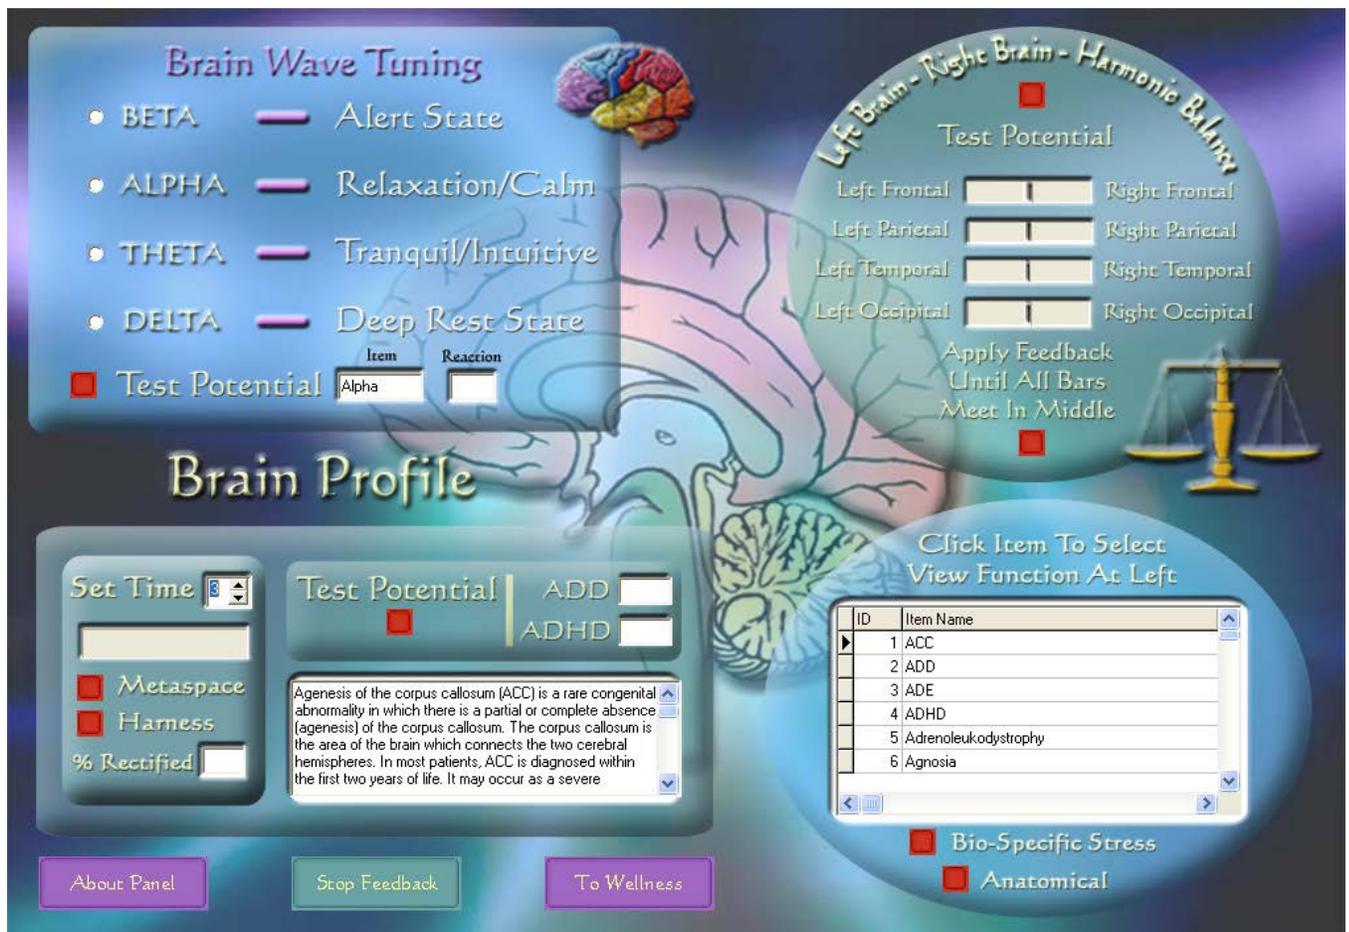

Neurology Panel - Brain Profile

Brain Wave Tuning: The Brain Wave Tuning program is located in the rectangular panel at the top left of the screen. To initiate the energetic reactivity process, click on the red **Test Potential** button. Upon completion, the results will be displayed in the two fields located at the bottom of this panel. The most reactive brain component will be displayed in the **Item** field. The client's reactivity response will be shown in the **Reaction** field. A response of 50% or greater may indicate an imbalance. A higher number represents a greater imbalance. To apply feedback, click on the lavender button next to the item you wish to address. Set the timer to the desired length of time (or use the 3-minute default). Click either the red **Metaspace** or **Harness** button to start the process. You may interrupt feedback by clicking the **Stop Feedback** button. Upon completion, check the **% Rectified** field located on the timer. A reading of 85% or greater is desirable.

Bio-Specific & Anatomical Panel: Located in the lower right corner is an oval graphic that contains a scrollable list of both **Bio-Specific** and **Anatomical** items. Click the red **Bio-Specific Stress** button to see a list of items that are specific to the system. Click the red **Anatomical** button to view a list of anatomical parts associated with the system.

By clicking on an item from either list, you will see a description of that condition in a dialog box to the left of the list. To apply feedback, click on an item to highlight it, set the timer to the desired length of time (unless you use the 3-minute default setting) and then click either the red [Metaspace](#) or [Harness](#) button to start. You may interrupt feedback by clicking the [Stop Feedback](#) button.

[ADD & ADHD Test](#): Located in the same rectangular panel as the timer, is the [Add & ADHD](#) assessment. Click on the red [Test Potential](#) button to activate the energetic evaluation. Reactivity results will be displayed in the two small fields to the right of the panel. A response of 50% or greater may indicate an imbalance. A higher number represents a greater imbalance. Feedback may be applied by clicking and highlighting either [ADD](#) or [ADHD](#) in the scrollable table. Then set the timer to the desired duration and click either [Metaspace](#) or [Harness](#) to initiate feedback.

[Left Brain – Right Brain Harmonic Balance](#): The round [Left Brain – Right Brain – Harmonic Balance](#) located in the upper right of the screen offers both testing and feedback features. To initiate the energetic testing process, click the red [Test Potential](#) button. Upon completion of the test, you may facilitate the balancing process by clicking the red button below the fields entitled, [Apply Feedback Until All Bars Meet in the Middle](#). This may take several repetitions. After the fifth try, the program will not respond and you must wait for a future session.

You may return to the main Wellness Info by clicking the [Wellness Info](#) button at any time.

Summary of Features:

Brain Wave Tuning:

- To initiate the energetic reactivity process, click on the red “Test Potential” button.
 - The most reactive brain component will be displayed in the “Item” field.
 - The client’s reactivity response will be shown in the “Reaction” field.
- To apply feedback click on the lavender button next to the item you wish to address.
- Set the timer to the desired length of time (or use the 3-minute default).
- Click either the red “Metaspace” or “Harness” button to start the process.
- Stop feedback by clicking the “Stop Feedback” button.

Bio-Specific & Anatomical Panel:


- Click the red “Bio-Specific Stress” button to see a list of conditions that are specific to the system.
- Click the red “Anatomical” button to see a list of anatomical parts associated with the system.
- To apply feedback, click on an item to highlight it, set the timer to the desired length of time (unless you use the 3-minute default setting) and then click either the red “Metaspace” or “Harness” button to start.
- You may interrupt feedback by clicking the “Stop Feedback” button.

ADD & ADHD Test:

- Click on the red “Test Potential” button to activate the energetic evaluation.
- Reactivity results will be displayed in the two small fields to the right of the panel.

Left Brain – Right Brain Harmonic Balance:

- To initiate the energetic testing process, click the red “Test Potential” button.
- To facilitate the balance process click the red button below the fields, entitled “Apply Feedback Until All Bars Meet in the Middle.”
- Repeat up to five times then discontinue.

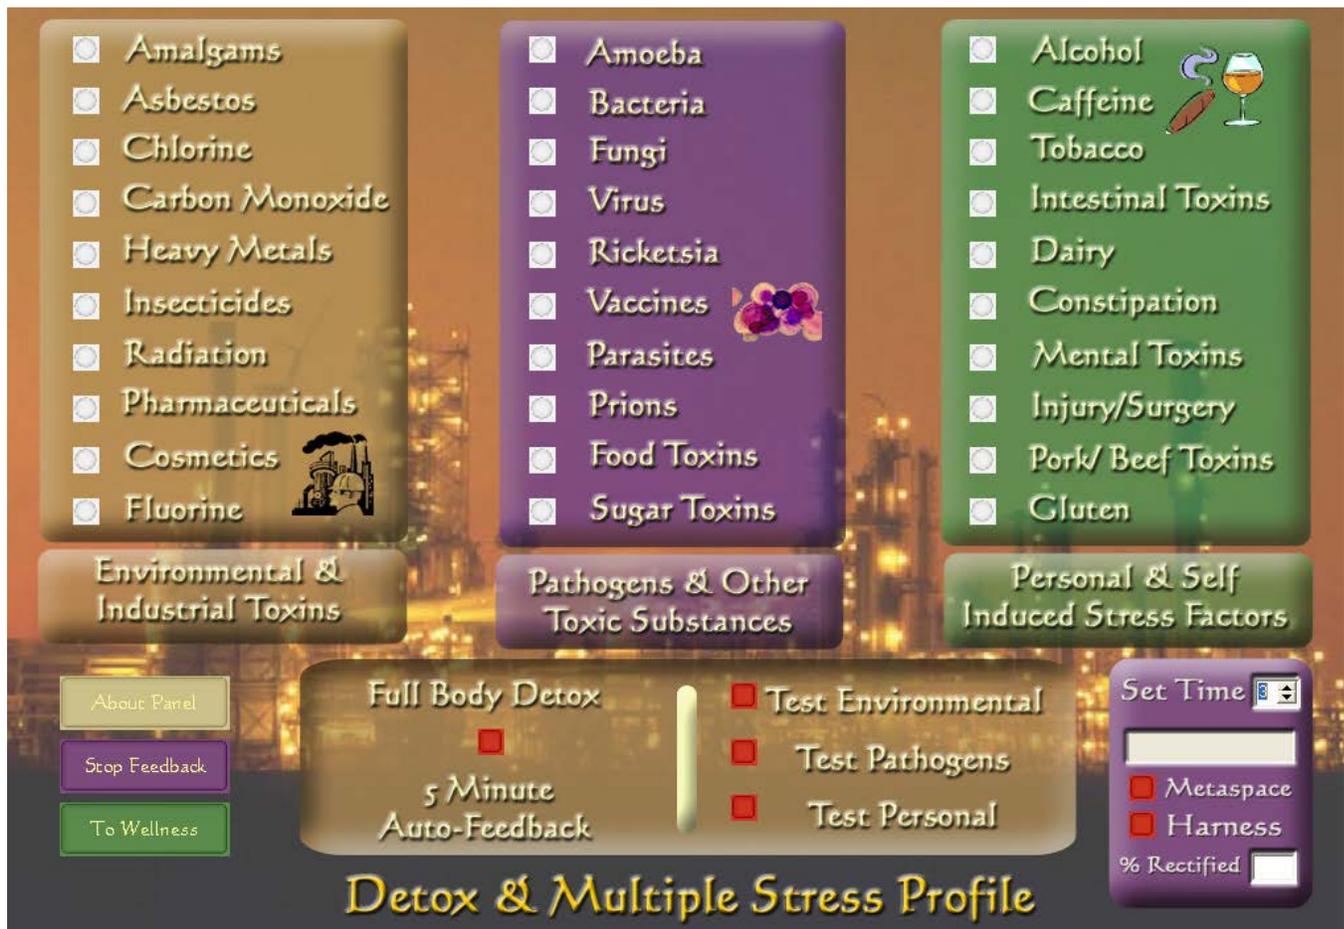

Detox & Multiple Stress Profile

Full Body Detox: To begin the **Full Body Detox** feedback process, click on the red button in the middle of the rectangular panel near the bottom of the screen. This will initiate an automated 5-minute process. A progress bar on the same panel will indicate when the process is complete. Typically this should be used **only once per visit**.

Test Environment, Test Pathogens and Test Personal: These features are found in the gold rectangular graphic at the lower middle of the screen. Click the red button next to any one of the three categories, to begin the assessment process. Upon completion, *the three highest, most reactive items*, within the selected panel will be displayed in red, yellow and blue respectively. To initiate the feedback process to the top three items, set the timer to the desired length, click either the red **Metaspace** or **Harness** button to start, and the program will automatically divide the time allotted and apply feedback to each of the three items in succession. You may interrupt feedback at any time by clicking the **Stop Feedback** button.

Additional Timed Feedback: You may apply feedback to any SINGLE item you choose in any of the three lists, by selecting *one item at a time*. Click the button next to the item chosen, then set the timer to the desired length (unless you choose to use the 3-minute default setting). Click either the red **Metaspace** or **Harness** button to enable the feedback process. You may interrupt feedback at any time by clicking the **Stop Feedback** button.

You may return to the main program list at any time by clicking the [Wellness Info](#) button

Summary of Features:

Full Body Detox:

- Click on the red, 5-Min. Auto Detox button in the middle of the rectangular panel near the bottom of the screen.
 - This will initiate an automated 5-minute process. A progress bar on the same panel will indicate when the process is complete.
 - This may be used *only once per visit*.

Test Environmental, Test Pathogens, Test Personal:

- Click the red Test button next to any one of these categories to begin the assessment process.
- The three highest and most reactive items, within the selected panel, will be displayed.
- Set the timer for the desired duration, and then click either Metaspace or Harness. You may interrupt feedback at any time by clicking the “Stop Feedback” button.

Additional Timed Feedback:

- You may apply feedback to any single item you choose in any of the three category lists, selecting *only one item at a time*.
- Click the button next to the item desired
- Set the timer to the desired length (unless you choose to use the 3-minute default)
- Click either the red “Metaspace” or “Harness” button to enable the feedback
- You may interrupt feedback at any time by clicking the “Stop Feedback” button.



PetVibes/Animal Profile

Type of Animal/Pet: To begin using this program, place a checkmark in one of the boxes next to the type of pet or animal you are balancing. The conditions that are specific to the type of pet you have chosen will appear in the **Specific Selections** area.

Specific Selections: There are a number of conditions pertinent to the pet or animal that appear in the **Specific Selections** panel. Scroll to the bio-specific item that is appropriate and highlight your selection. Click the red button to the right of the panel to initiate a 1-minute auto-feedback procedure. For extended feedback, set the timer for the desired length (unless you choose to use the 3-minute default setting). Click either the red **Metaspace** or **Harness** button to start feedback. You may discontinue feedback, at any time, by clicking the **Stop Feedback** button. You may balance only one item at a time.

The lower portion of the rectangular graphic contains four **Add Emphasis** boxes that include the add-on features of: **Inflammation**, **Infection**, **Degeneration** and **Pain**. Any or all of these boxes may be selected along with any single feedback item of choice.

You may return to the main program list at any time by clicking [Wellness Info](#).

Summary of Features:

- Place a checkmark next to the type of animal to be evaluated
- Scroll through the “Specific Selections” box and highlight your selection
 - Option: Check any or all of the four “Add Emphasis” buttons
- Click the red button to the right of the panel to initiate a 1-minute auto-feedback procedure.
- For extended feedback, click set the timer to the desired length (unless you choose to use the 3-minute default setting)
- Click either the red “Metaspace” or “Harness” button to start feedback.
 - Option: You may discontinue feedback by clicking the ‘Stop Feedback’ button.

System Specifications

The I.M.A.E.T. System is a complete unit containing a Program CD, interface box, head and limb harnesses, and a USB cable that connects the interface box to the computer.

The I.M.A.E.T. system software is fully [Windows XP & Windows Vista](#) compatible and are the required operating systems. A Pentium 4, AMD or equivalent processor, operating at 1.5 Ghz or greater, containing a minimum 1 gigabyte of RAM and ample hard drive capacity is recommended. [A USB port](#) is essential. Although Celeron, Duron and Centrino processors may be functional *they are not recommended, since they are extremely slow processors*. The program is written to operate at [1024 X 768 screen resolution](#). If using a laptop, a 15” screen, or larger, is highly advantageous.

The I.M.A.E.T. System is a biofeedback/relaxation management device. All hardware and software components are warranted for one full year against manufacturing defects. Tech support will be provided, free of charge, for 90 days following delivery. Such support will pertain to I.M.A.E.T. System hardware or software problems only. [It does not include support relevant to training issues, use or setup of your computer system, Microsoft Windows operating systems, scanners or other unrelated issues.](#) **Please Note: You must contact your computer specialist for setup and use of the I.M.A.E.T. System software related to Windows or internet.**

Software upgrades will be released subject to a \$50.00 manufacturing, shipping and handling fee, which may vary somewhat in the future. (Major upgrades may incur a higher fee) The software will be upgraded periodically with new and innovative features. Hardware upgrades may require either a flat-rate or pro-rated fee, to be determined by BioGen Technologies.

All of the program tables, items and/or substances, encoded within the software have been independently developed or purchased by this company or are otherwise public domain.

The reactivity process, entrainment loop, feedback and safety mechanisms used within the I.M.A.E.T. System are exclusive and proprietary.

Answers To A Few Commonly Asked Questions

Yes, the signature of any external item may be imported into the Personal Substance table (Biofield Test page), Nutrition table or Homeopathic matrix from the tray situated on top of the interface device.

Yes, the I.M.A.E.T. system does provide a distance feedback mode called “Metaspace” for use with all modalities, as well as the typical harness interface connection.

No, the I.M.A.E.T. system software will **NOT** operate through any other interface box. Nor will other software programs function through the I.M.A.E.T. system device.

Yes, the I.M.A.E.T. system does provide an “entrainment or auto-monitoring loop” associated with all its assessment and feedback modalities.

Yes, the System provides built-in EMR (Electro-Magnetic Radiation) program which may be activated by the technician.

Yes, the I.M.A.E.T. System provides well over 100 channels of information and uses proprietary tri-vector technology and reactivity processes. [Please understand that technical information surrounding this process will not be revealed by the manufacturer.](#)

Yes, the I.M.A.E.T. System interface box does provide the latest safety isolation components.

Batteries are NOT necessary for the use of the I.M.A.E.T. System Interface box. Power is received from the computer by way of the supplied USB cable.

It is highly recommended that similar programs, or those requiring a user code that, [locks onto the hard drive](#), should not be loaded onto the same computer. All other commonly used commercial software programs are perfectly compatible and acceptable.

Technical Support, Customer and Educational Services

The I.M.A.E.T. System hardware and software are warranted for one full year following the date of purchase. Please do not tamper with or open the interface box.

Please Note: The interface box has been provided with an internal security seal. If the device has been opened and the seal broken, the warranty will not be honored.

For **Customer Service**, please contact BioGen Technologies at biogenbiofeedback@gmail.com or call 315-430 4211.

For **Technical Support**, please contact BioGen Technologies at biogenbiofeedback@gmail.com or call 315-430 4211.

For **Educational Information**, please contact www.imaet.com

Our sincerest thanks and gratitude,

BioGen Technologies ^{INC}

IMPLEMENTING THE NAET PROTOCOL WITH THE IMAET:

Analysis of the patient or testing the database:

There are 4 different ways of analyzing/testing your patient with the IMAET. The choice depends on expediency, details of patient history and clinician's preference.

1) 1 – CHANNEL ANALYSIS

Patient places one hand on the contact plate of the interface box. Disconnect the harness. See picture below.

Calibrate on the wellness profile, save, upload database (biofield test), go to wellness info and select NAET. Choose the Basic Panel or the full NAET Test Panel and run the test.

Note: This is the equivalent of holding a vial in your hand.



2) 9 - CHANNEL ANALYSIS

Place the head harness on patient's forehead as shown below. 8 contacts are touching skin on forehead. Gently wrap the strap around patients head and velcro in back of the head. The patient places one hand on the contact plate of the interface box. Calibrate on the wellness profile, save, upload database (biofield test), go to wellness info and select NAET. Choose the Basic Panel or the full NAET Test Panel and run the test.



8-channel harness contact points are placed over forehead of the patient, intercepting the 8 meridians transverse the human skull.

3) 12 – CHANNEL ANALYSIS

This is the most complete analysis method, measuring all 12 meridians of the body. As shown in the picture below, the patient is “hooked up” to the full interface harness. No hand is placed on the interface box!

Calibrate on the wellness profile, save, upload database (biofield test), go to wellness info and select NAET. Choose the Basic Panel or the full NAET Test Panel and run the test.

Note: This method represents the deepest and most accurate analysis.



4) METASPACE

No direct contact with the patient. No interface between computer and patient.

Go to the NAET panel and choose the Basic Panel (first 3 NAET kits) or the top panel, which contains 23 NAET kits. Interface box not plugged in.

Note: This mode appropriate on patients with pacemakers and defibrillators or long distance operation (Virtual Mode).

It's best to use this feature from the start.

1) Unplug the interface box before entering the IMAET program.

2) Enter the program as usual.

3) A window will pop up, asking whether to continue in Virtual Mode.

Click YES. You are now automatically for the entire session in metaspace mode.

4) METASPACE

No direct contact with the patient. No interface between computer and patient.

Go to the NAET panel and choose the Basic Panel (first 3 NAET kits) or the top panel, which contains 23 NAET kits. Interface box not plugged in.

Note: This mode appropriate on patients with pacemakers and defibrillators or long distance operation (Virtual Mode).

It's best to use this feature from the start.

1) Unplug the interface box before entering the IMAET program.

2) Enter the program as usual.

3) A window will pop up, asking whether to continue in Virtual Mode.

Click YES. You are now automatically for the entire session in metaspace mode.